


CUSTOMER PROVIDED:

RECEPTACLES:



- OUTLET "A": Outlet, Shall be for the Bone Density Machine, dedicated circuit, 120 volts 20 amps. NEMA 5-20R Dedicated (AS PER LOCAL CODE)
- OUTLET "B": Network drop and telecommunication outlet and Power Outlet for Computer & Printer. 120 volts 20 amps.

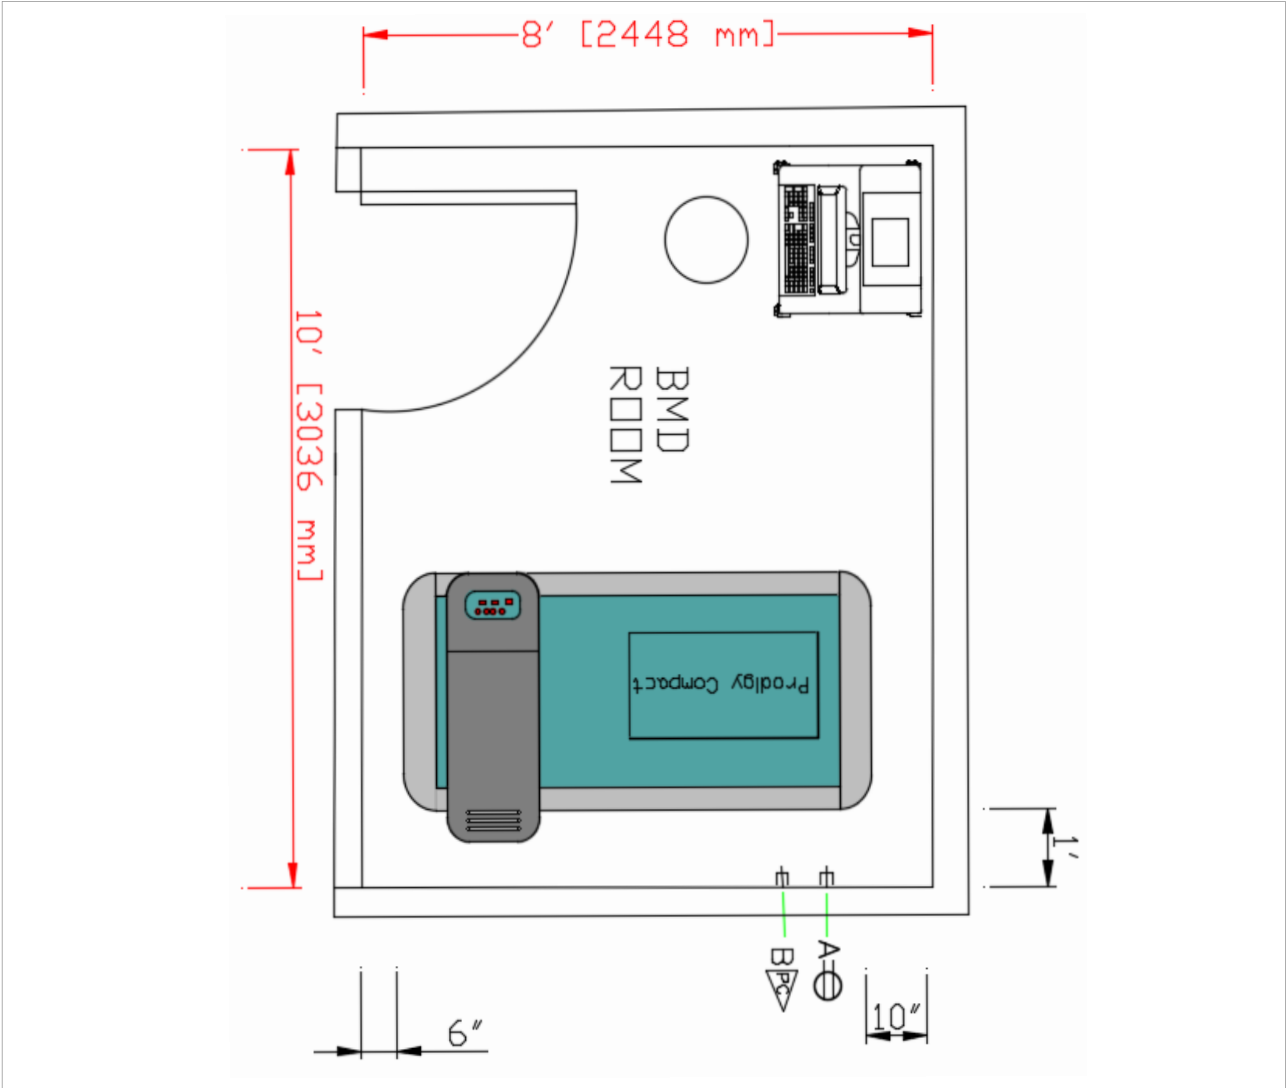

BMD ROOM

ALL DIMENSIONS = IMPERIAL / [METRIC]

TRUE NORTH

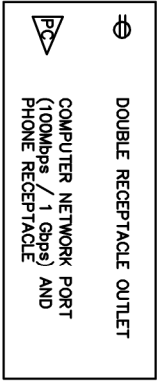

COMPACT PRODIGY BMD – ROOM LAYOUT

Optimum Sample 10' X 8' Room

Aymes Medical
Date Prepared: Sample Drawing