



CUSTOMER PROVIDED:

RECEPTACLES:

- OUTLET "A": Outlet, Shall be for the Bone Density Machine, dedicated circuit, 120 volts 20 amps. NEMA 5-20R Dedicated (AS PER LOCAL CODE)
- OUTLET "B": Network drop and telecommunication outlet and Power Outlet for Computer & Printer. 120 volts 20 amps.

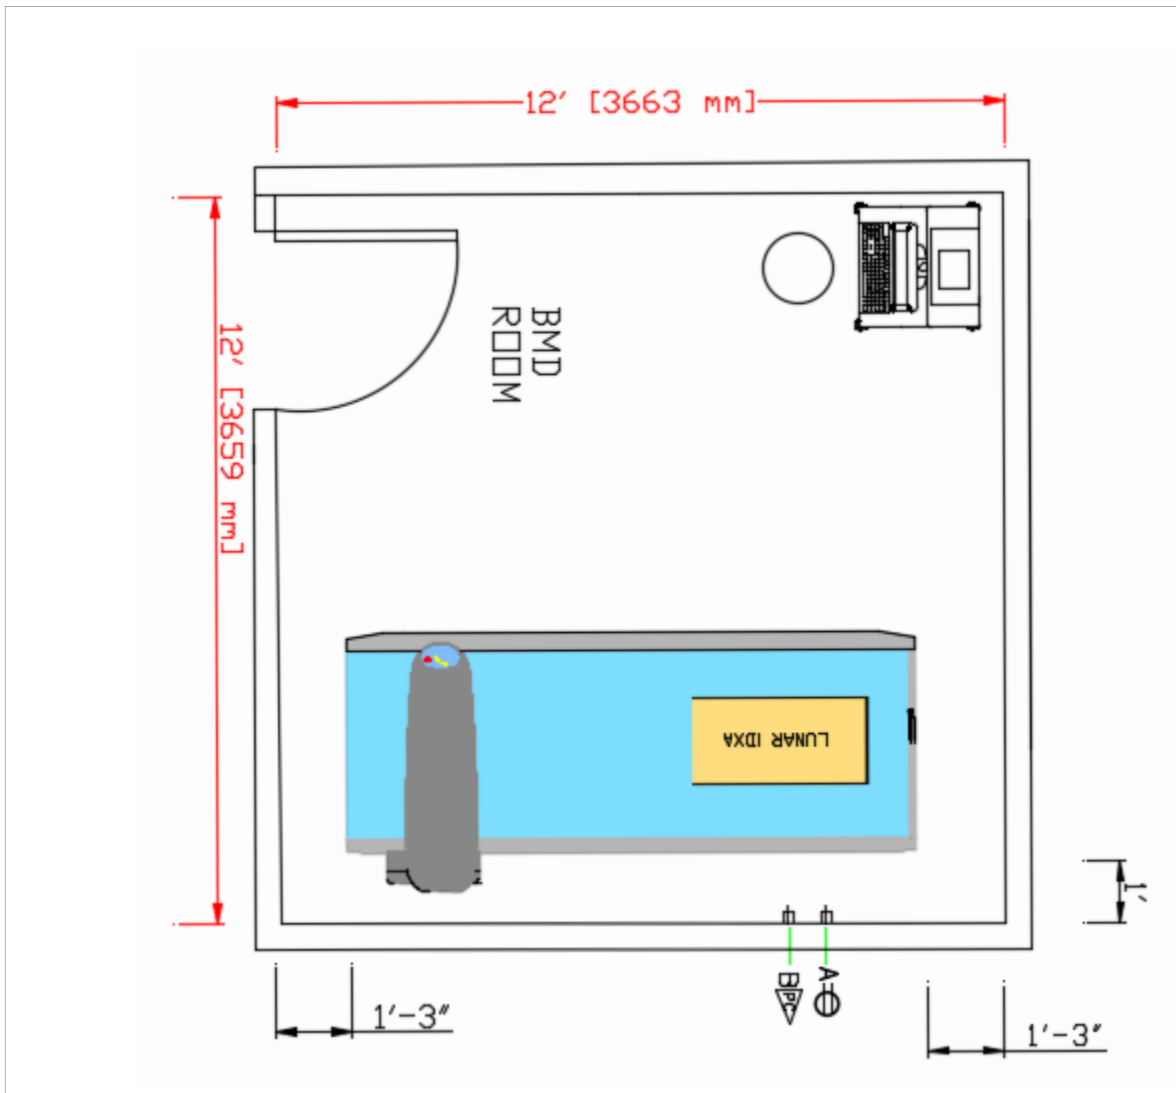

IDXA – ROOM LAYOUT

Minimum Sample 12' X 12' Room

Aymes Medical
Date Prepared: Sample Drawing

BMD ROOM

ALL DIMENSIONS = IMPERIAL / [METRIC]